

CORRECTION


Hecht HS

Coronary Artery Calcium Scanning: Past, Present, and Future.

J Am Coll Cardiol Img 2015;8:579-96.



In Figure 4, the numbers above the “CACS > 400” columns are identical to those above the “CACS 101-400” columns. The correct figure is printed below and has also been corrected online.

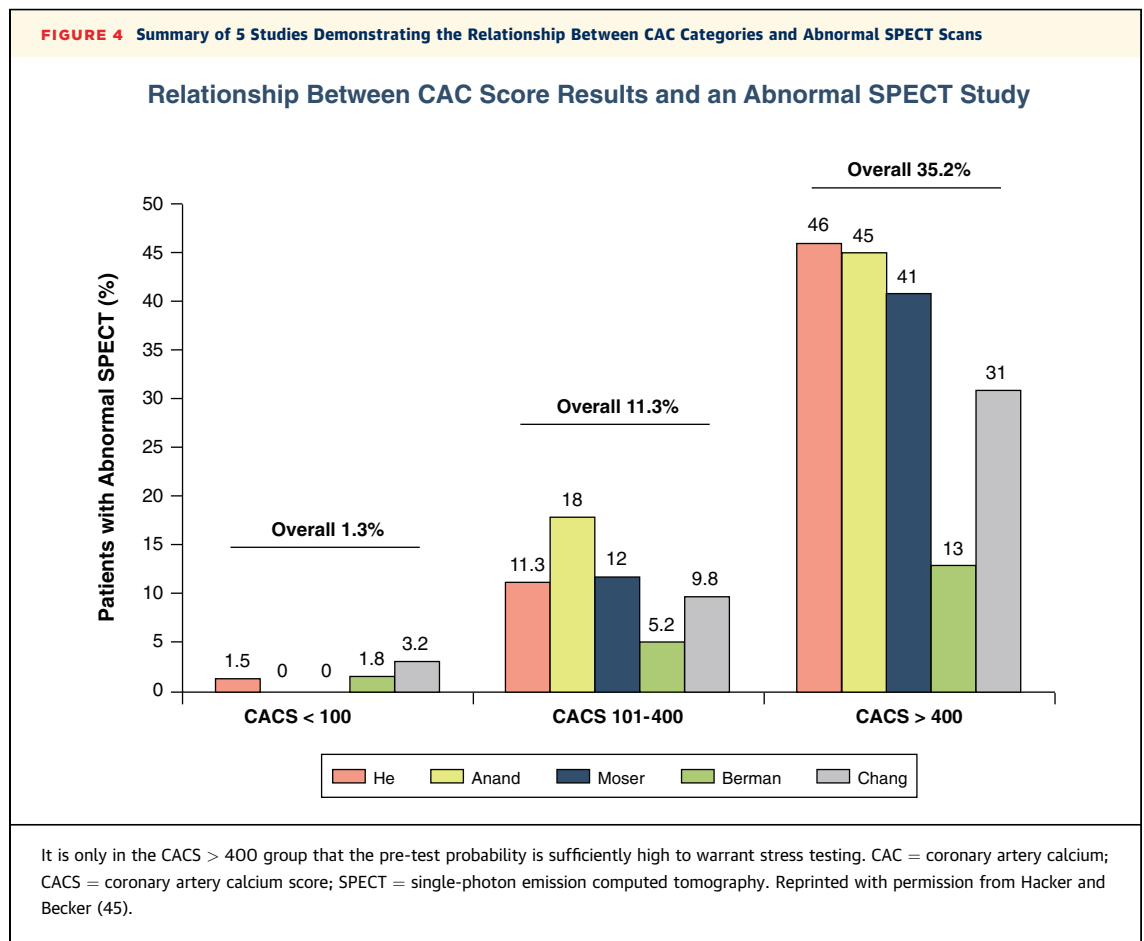

<http://dx.doi.org/10.1016/j.jcmg.2015.07.001>